

**AeroChamber**  
*Plus* with **Flow-Vu**  
Valved Holding Chamber

**Easy to Use... Easy to Learn... Most Preferred.<sup>1</sup>**



*"Face mask seal is critical for efficient ventilation and aerosol delivery through holding chamber devices"<sup>2</sup>*

**ComfortSeal\* Mask Sizer**

SMALL - INFANT

MEDIUM - CHILD

LARGE - ADULT

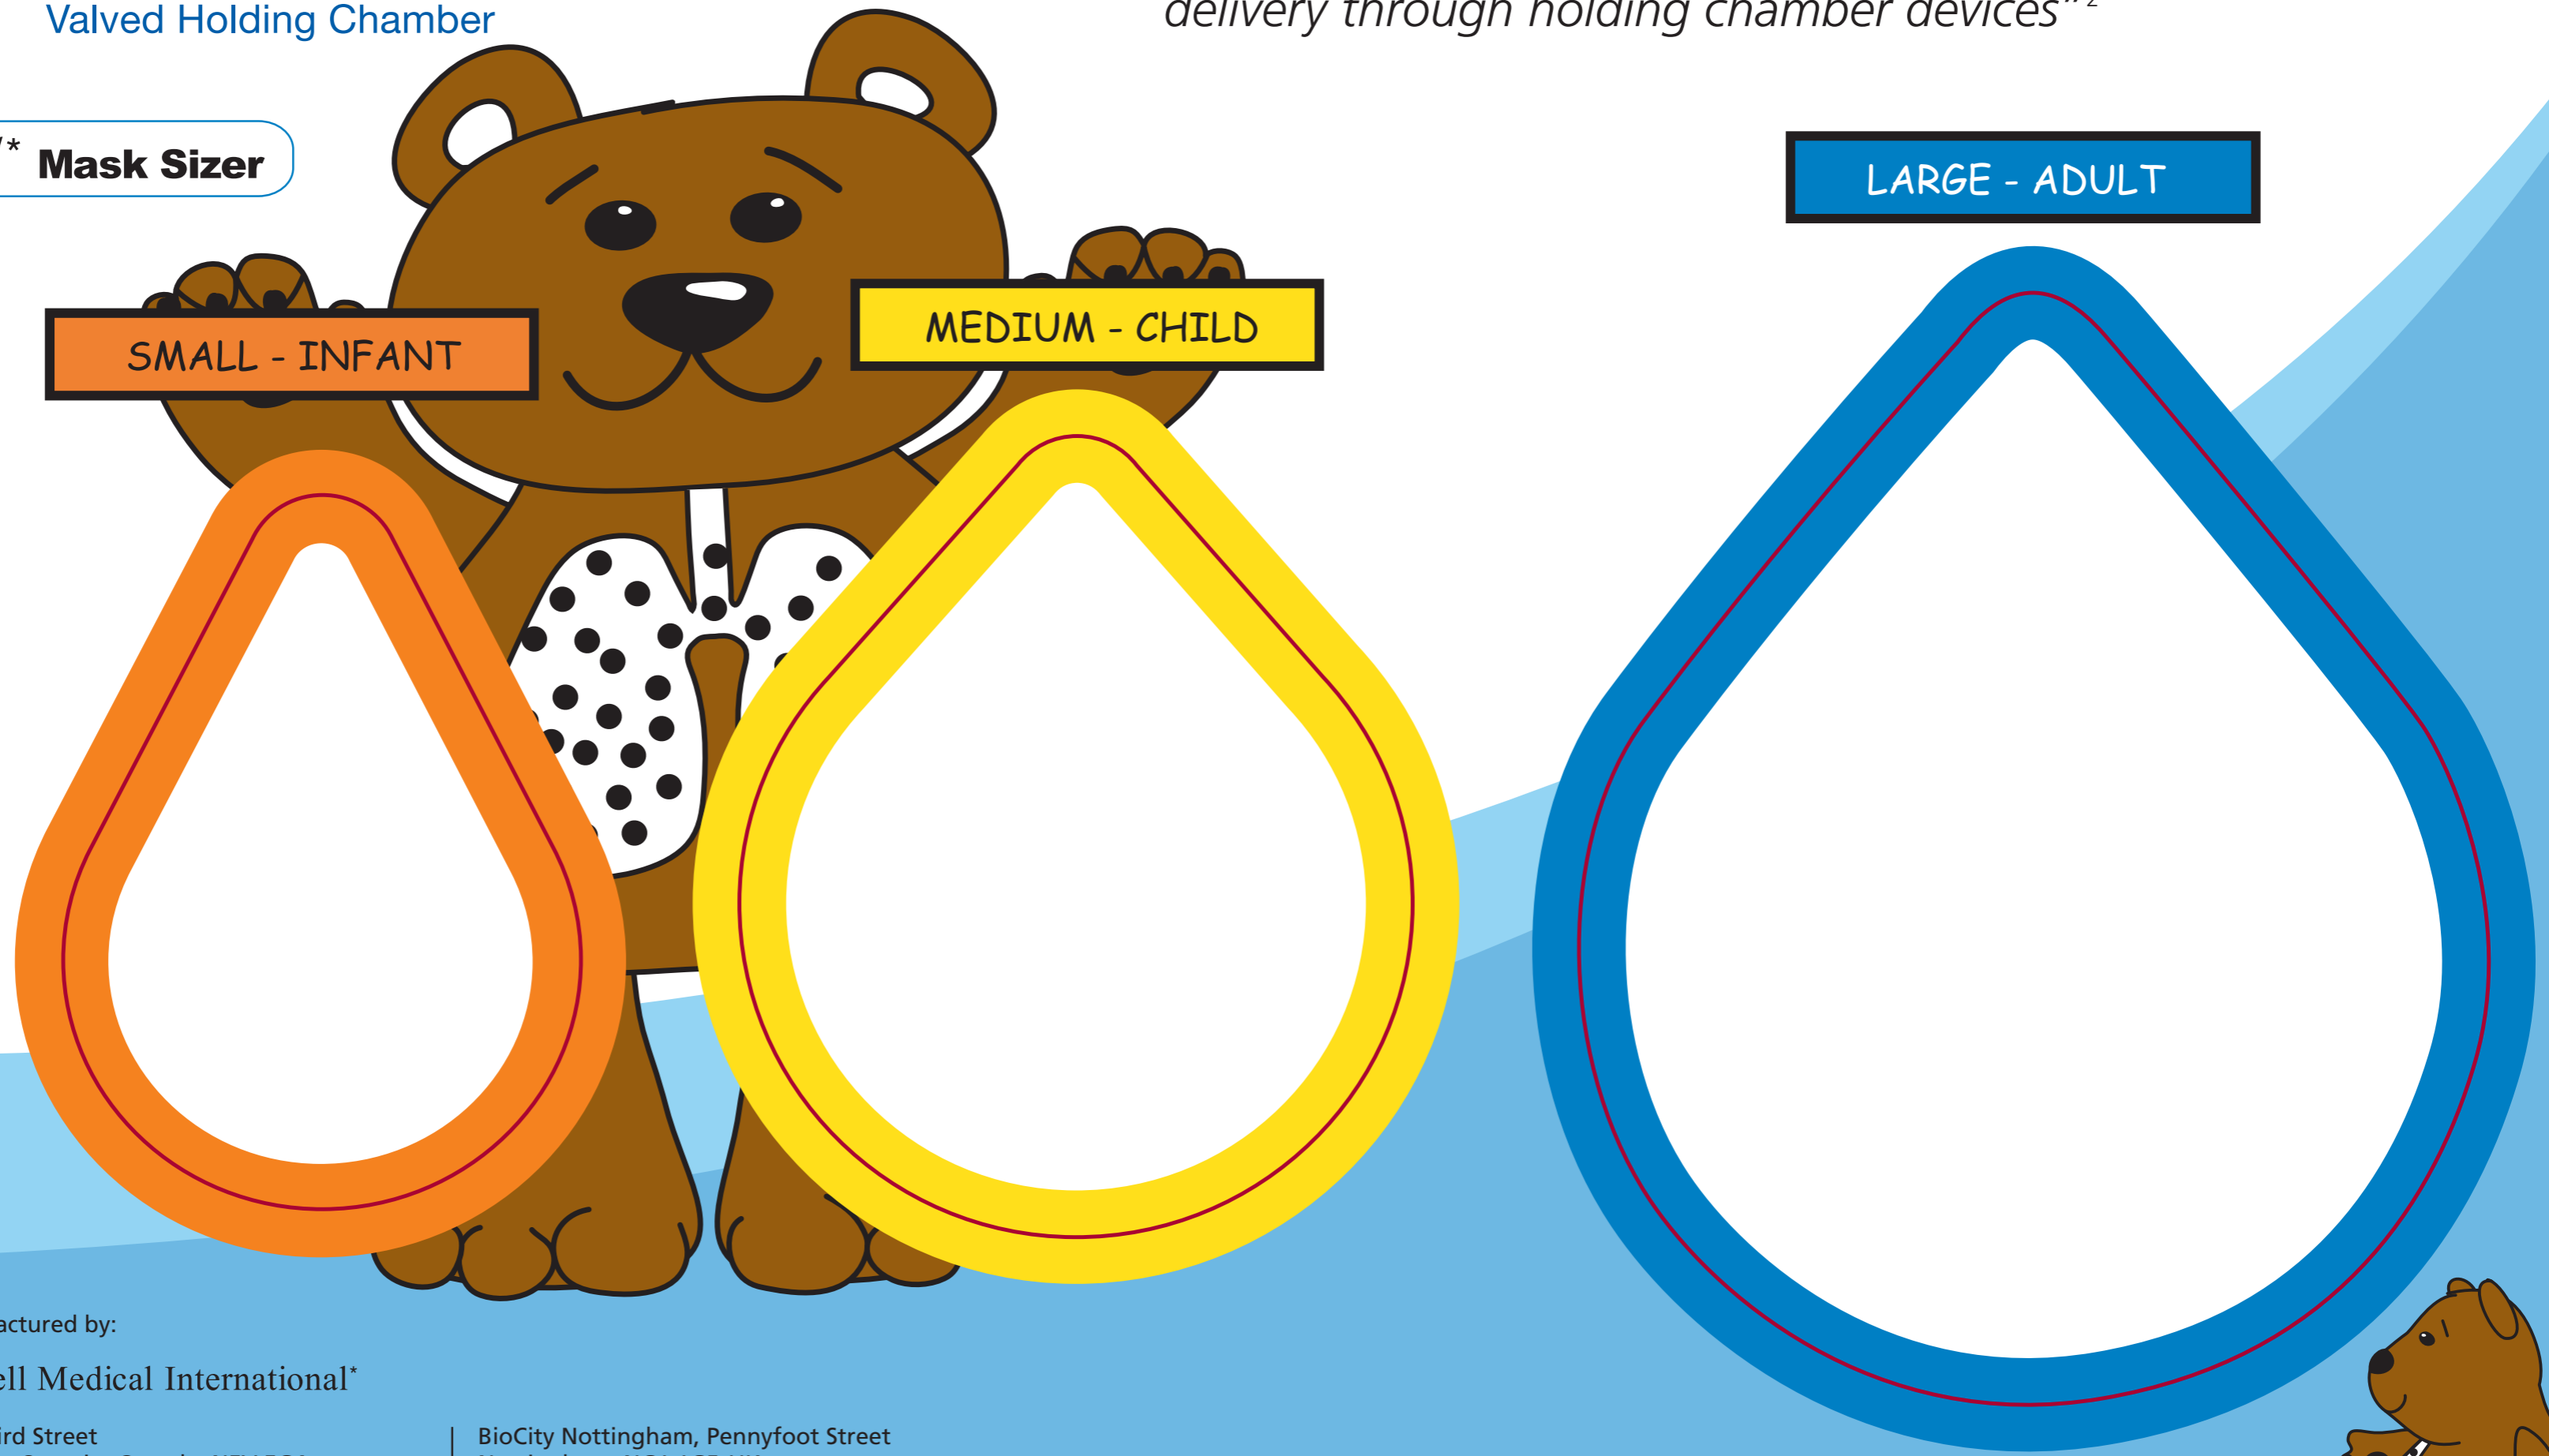

Manufactured by:

**Trudell Medical International\***

725 Third Street  
London, Ontario, Canada, N5V 5G4  
Phone: +1-519-455-7060 Fax: +1-519-455-7858  
Email: customerservice@trudellmed.com

BioCity Nottingham, Pennyfoot Street  
Nottingham, NG1 1GF, UK  
Tel: +44 115 912 4380  
Fax: +44 115 912 4289

[www.trudellmed.com](http://www.trudellmed.com)



\*


# AeroChamber<sup>®</sup>

Plus<sup>\*</sup> with Flow-Vu<sup>\*</sup>

Valved Holding Chamber

Easy to **Use**... Easy to **Learn**... **Most Preferred**.<sup>1</sup>

For better asthma management, check and record your Peak Expiratory Flow Rate (PEFR) with a **TruZone<sup>®</sup>** Peak Flow Meter.



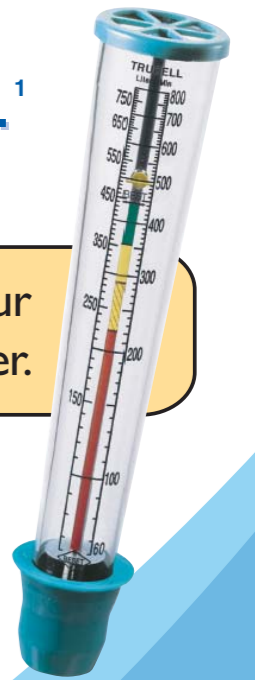


LARGE - ADULT

ComfortSeal<sup>\*</sup> Mask Sizer

MEDIUM - CHILD

SMALL - INFANT

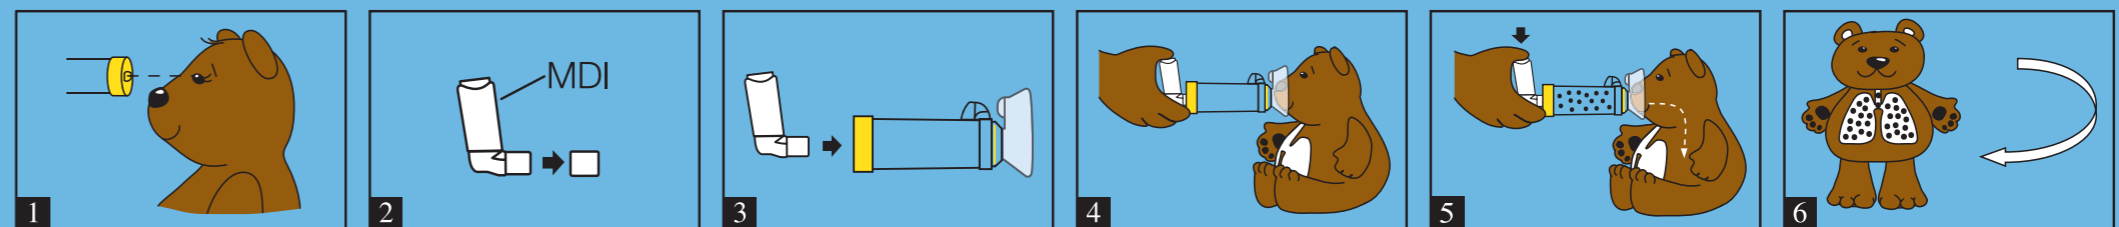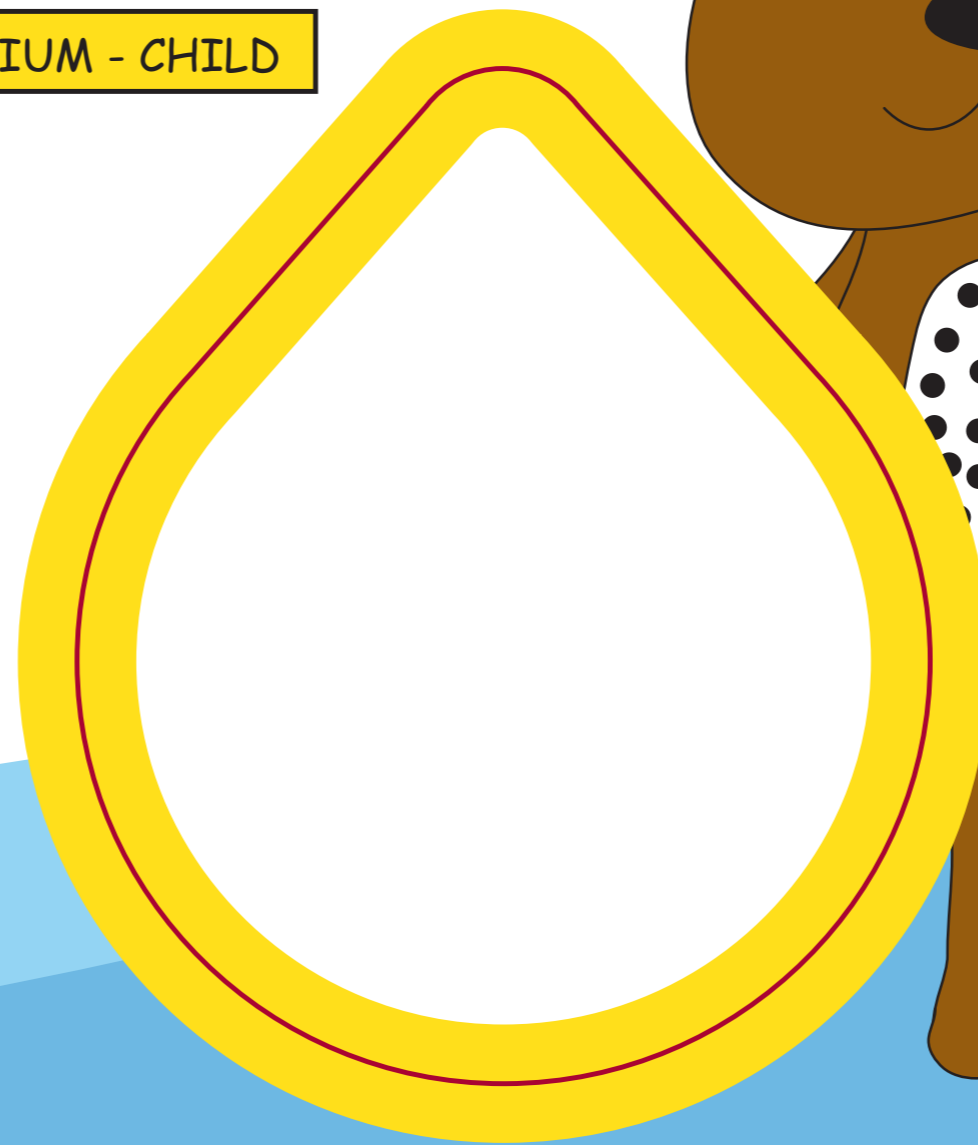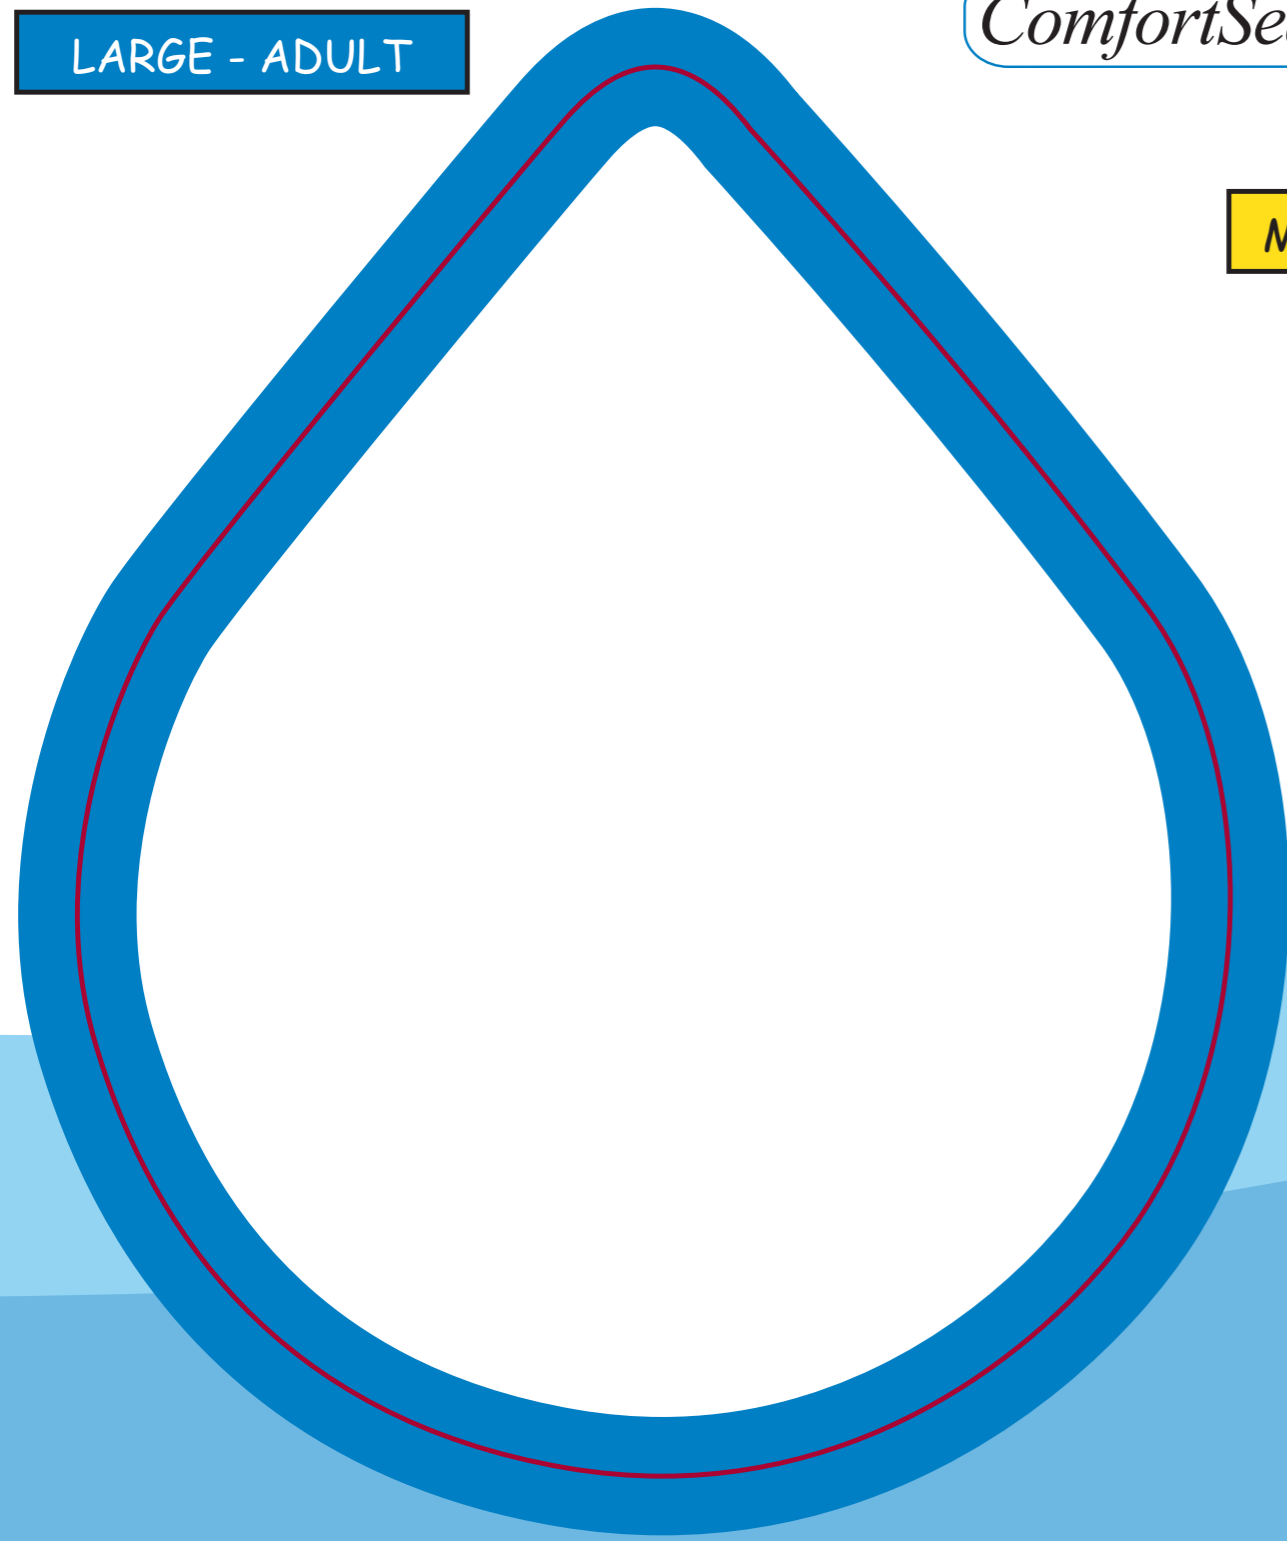

<sup>1</sup> NOP Healthcare, UK, March 2000. <sup>2</sup> "Delivery of Aerosols to Children with MDI and Holding Chambers (MHC) is Critically Dependent on the Facemask Seal" Amirav et al, study presented at the ALA/ATS May 1999. 10101-001 Rev A. Printed in Canada. \* trade marks and registered trade marks of Trudell Medical International. Copyright © Trudell Medical International 2006. All rights reserved.